




R. M. Young Company
Barometric Pressure Sensor Calibration Record
Serial Number: BPA4180
Calibration Date: January 28, 2012

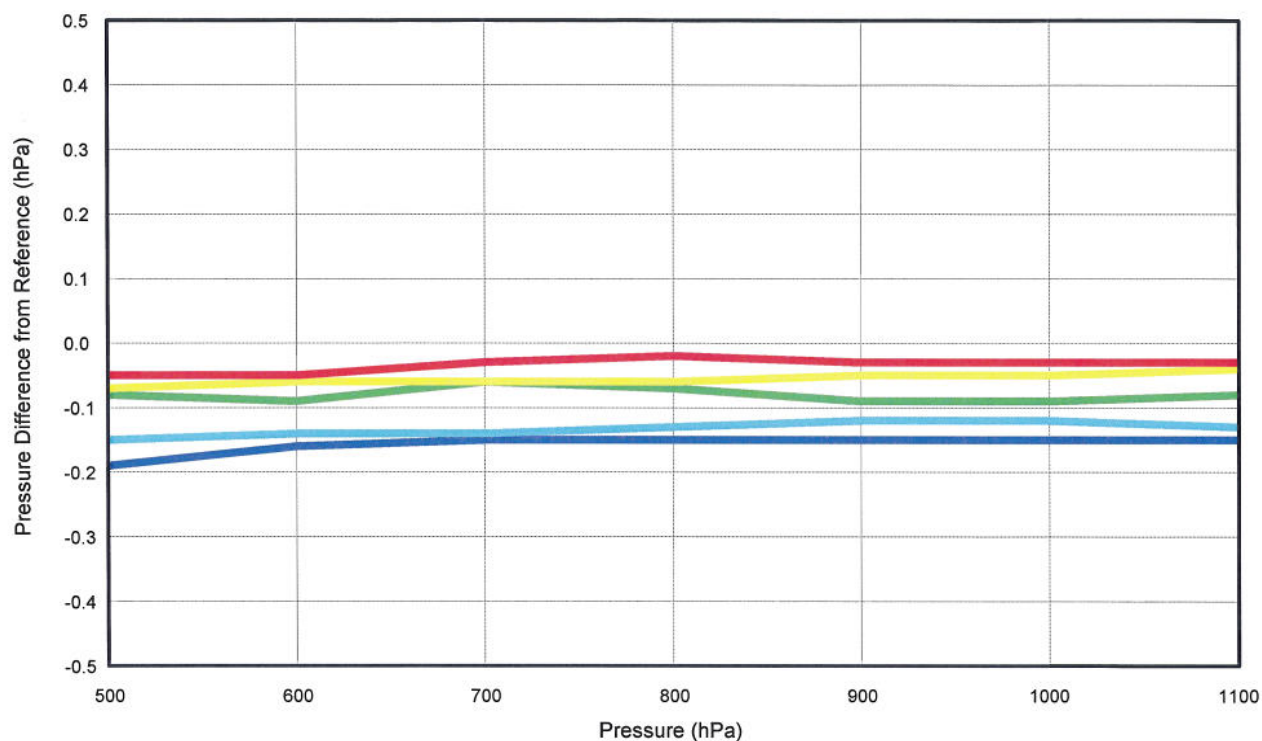

LEGEND:

-40°C —
-25°C —
0°C —
25°C —
60°C —

Sensor calibration checked from 500 to 1100 hPa in 100 hPa increments at 5 temperatures.
Pressure reference traceable to NIST.

Average Difference from Pressure Reference: -0.09 hPa
Standard Deviation: 0.05 hPa

YOUNG USA

BAROMETRIC PRESSURE SENSOR

MODEL: 61302V

RANGE: 500-1100 hPa

OUTPUT: 0-5 VDC, RS232

SUPPLY: 7-30 VDC

S.N.: BPA4180



TRIG / RX

REF

- PWR

+ PWR

VOUT / TX

